



DS Implants™

DS PrimeTaper® Implant System

Surgical product catalog





Products specifically designed for use with the PrimeTaper EV Implants are presented in this product catalog. For additional products, please refer to the product catalog for Astra Tech Implant System EV. For more information visit www.dentsplysirona.com

All Dentsply Sirona Instructions for Use are available on www.dentsplysirona.com/ifu

All products may not be regulatory cleared/released/licensed in all markets. Please contact the local Dentsply Sirona sales office for current product assortment and availability.

To improve readability for our customers, Dentsply Sirona does not use ® or ™ in body copy. However, Dentsply Sirona does not waive any right to the trademark and nothing herein shall be interpreted to the contrary.

Product illustrations are not to scale.



CONTENTS

| | |
|--|----|
| 1. Implant packaging | 4 |
| Color coding | 4 |
| 2. Implants | 5 |
| 3. Cover screws | 6 |
| 4. Healing abutments | 6 |
| 5. Instruments | 8 |
| Initial drills | 8 |
| Drills | 8 |
| Screw taps | 9 |
| Intermediate drills | 9 |
| 6. Trays | 10 |
| 7. Other surgical instruments | 13 |
| 8. Instruments - Guided surgery | 15 |
| Punches | 15 |
| Drills | 15 |
| Intermediate drills | 17 |
| Taps | 17 |
| Sleeves | 18 |
| Driver | 18 |
| Stabilization Abutment | 19 |
| Guide Fixation | 19 |
| Surgical Tray | 19 |
| 9. Material specifications | 21 |
| 10. Index | 22 |

1. Implant packaging

PrimeTaper EV implants are supplied in a blister container with an outer box.



Outer box package

- Implant diameter, specific color coding according to EV connection and implant length information on side labels.
- QR codes accessible on two sides.
- Stackable, all important product information remains visible.
- Instructions For Use (IFU) available electronically (eIFU): ifu.dentsplysirona.com

Blister

- Inner sterile package
- Contains implant container
- Peel-off label with batch code supporting a convenient documentation of the treatment.

Color coding

The DS PrimeTaper Implant line is available in different diameters and lengths. The color coding makes it easy to identify the correct connection and to select the right prosthetic components.

| Implant Ø mm | 3.0 | 3.6 | 4.2 | 4.8 | 5.4 |
|--------------|-----|-----|-----|-----|-----|
| Connections | XS | S | M | L | L |
| Lengths mm | - | - | 6.5 | 6.5 | 6.5 |
| | 8 | 8 | 8 | 8 | 8 |
| | 9 | 9 | 9 | 9 | 9 |
| | 11 | 11 | 11 | 11 | 11 |
| | 13 | 13 | 13 | 13 | 13 |
| | 15 | 15 | 15 | 15 | 15 |
| | - | 17 | 17 | 17 | - |

2. Implants

XS PrimeTaper EV Ø3.0



| | | | | | |
|-----------|----------|----------|----------|----------|----------|
| Length mm | 8 | 9 | 11 | 13 | 15 |
| Order No. | 68011085 | 68011086 | 68011087 | 68011088 | 68011089 |

S PrimeTaper EV Ø3.6



| | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|
| Length mm | 8 | 9 | 11 | 13 | 15 | 17 |
| Order No. | 68011090 | 68011091 | 68011092 | 68011093 | 68011094 | 68011095 |

M PrimeTaper EV Ø4.2



| | | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|----------|
| Length mm | 6.5 | 8 | 9 | 11 | 13 | 15 | 17 |
| Order No. | 68011096 | 68011097 | 68011098 | 68011099 | 68011100 | 68011101 | 68011102 |

L PrimeTaper EV Ø4.8



| | | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|----------|
| Length mm | 6.5 | 8 | 9 | 11 | 13 | 15 | 17 |
| Order No. | 68011103 | 68011104 | 68011105 | 68011106 | 68011107 | 68011108 | 68011109 |

L PrimeTaper EV Ø5.4




| | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|
| Length mm | 6.5 | 8 | 9 | 11 | 13 | 15 |
| Order No. | 68011110 | 68011111 | 68011112 | 68011113 | 68011114 | 68011115 |

PrimeTaper EV

Titanium¹, sterile

- The implants are available in a versatile range of diameters and lengths for all indications, including situations with limited space and/or bone quantity.



XS

S

M

L

- Specific colors have been assigned to the different implant-abutment connection sizes and are consistently used throughout the system
- OsseoSpeed surface treatment over the entire implant including the micro threads up to the bevel
- Compatible with the restorative assortment with the EV connection

3. Cover screws

Cover Screw EV

Titanium alloy², sterile

Cover Screw EV


| | | | | |
|-----------|---|---|---|---|
| |  |  |  |  |
| | XS | S | M | L |
| Order No. | 68010001 | 68010002 | 68010005 | 68010006 |

4. Healing abutments





Healing Abutment EV

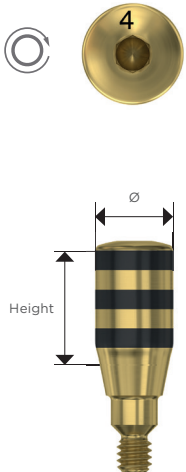Titanium alloy², sterile





- For soft tissue sculpturing during the healing phase
- Color coded and marked with height
- Laser-marked bands for showing height




XS Healing Abutment EV

| | | | | |
|-----------|---|---|---|---|
| |  |  |  |  |
| Ø mm | 4 | 4 | 4 | 4 |
| Height mm | 2 | 3 | 4 | 6 |
| Order No. | 68013044 | 68013045 | 68013046 | 68013047 |





S Healing Abutment EV

| | | | | |
|-----------|---|---|---|---|
| |  |  |  |  |
| Ø mm | 4 | 4 | 4 | 4 |
| Height mm | 2 | 3 | 4 | 6 |
| Order No. | 68013048 | 68013049 | 68013050 | 68013051 |

M Healing Abutment EV

| | | | | |
|-----------|---|---|---|---|
| |  |  |  |  |
| Ø mm | 4 | 4 | 4 | 4 |
| Height mm | 2 | 3 | 4 | 6 |
| Order No. | 68013052 | 68013053 | 68013054 | 68013055 |


L Healing Abutment EV

| | | | | |
|-----------|---|---|---|---|
| |  |  |  |  |
| Ø mm | 4.3 | 4.3 | 4.3 | 4.3 |
| Height mm | 2 | 3 | 4 | 6 |
| Order No. | 68013056 | 68013057 | 68013058 | 68013059 |

HealDesign™ EV

Titanium alloy², sterile

- For soft tissue sculpturing during the healing phase
- Can be used for both one- and two-stage surgery
- Marked with diameter and height

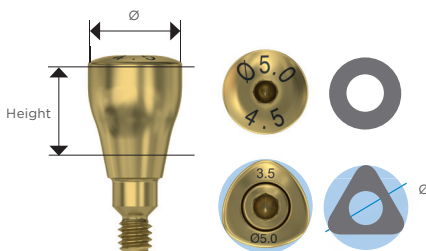

Round shapes are indicated for all positions in the mouth.

Triangular shapes are indicated for anterior implant sites to mimic the incisors and canines. The Triangular HealDesign EV is a two-piece abutment.

XS HealDesign EV



| | | | | |
|-----------|----------|----------|----------|----------|
| ∅ mm | 3.5 | 3.5 | 3.5 | 3.5 |
| Height mm | 2.5 | 3.5 | 4.5 | 6.5 |
| Order No. | 68013001 | 68013002 | 68013003 | 68013004 |

S HealDesign EV



| | | | | | | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|
| ∅ mm | 4 | 4 | 4 | 4 | 5 | 5 | 5 | 5 | 6 | 6 | 5 |
| Height mm | 2.5 | 3.5 | 4.5 | 6.5 | 2.5 | 3.5 | 4.5 | 6.5 | 3.5 | 4.5 | 3.5 |
| Order No. | 68013005 | 68013006 | 68013007 | 68013008 | 68013009 | 68013010 | 68013011 | 68013012 | 68013013 | 68013014 | 68013039 |

M HealDesign EV



| | | | | | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|
| ∅ mm | 5 | 5 | 5 | 5 | 6.5 | 6.5 | 6.5 | 6.5 | 5 | 6.5 |
| Height mm | 2.5 | 3.5 | 4.5 | 6.5 | 2.5 | 3.5 | 4.5 | 6.5 | 3.5 | 3.5 |
| Order No. | 68013015 | 68013016 | 68013017 | 68013018 | 68013019 | 68013020 | 68013021 | 68013022 | 68013040 | 68013041 |

L HealDesign EV



| | | | | | | | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|
| ∅ mm | 5 | 5 | 5 | 5 | 6.5 | 6.5 | 6.5 | 6.5 | 7.5 | 7.5 | 5 | 6.5 |
| Height mm | 2.5 | 3.5 | 4.5 | 6.5 | 2.5 | 3.5 | 4.5 | 6.5 | 3.5 | 4.5 | 3.5 | 3.5 |
| Order No. | 68013023 | 68013024 | 68013025 | 68013026 | 68013027 | 68013028 | 68013029 | 68013030 | 68013031 | 68013032 | 68013042 | 68013043 |

5. Instruments

Initial drills

Stainless steel¹, sterile

- Multiple use with option for single use except for the Precision Drill, which is for single use only
- Used to mark a starting point

The Precision Drill is an extremely sharp drill and should be handled with caution to avoid injury.

Guide Drill



Precision Drill



| | | |
|-----------|----------|----------|
| Ø mm | n/a | n/a |
| Order No. | 68015133 | 68015134 |

Drills


PrimeTaper Drill

Stainless steel¹, TiN-coated², sterile

- Laser-marked depth indication lines
- Multiple use with option for single use
- Marked with numbers 1-7

Drilling depth

- The drilling depth is measured from the widest part of the drill tip up to the indication line
- Additional tip depth is maximum 1.0 mm regardless of the diameter of the drill

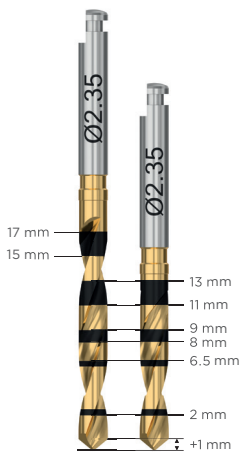

Short



| | | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|----------|
| Ø mm | 1.9 | 2.35 | 2.95 | 3.55 | 4.15 | 4.75 | 5.35 |
| Order No. | 68015324 | 68015325 | 68015326 | 68015327 | 68015328 | 68015329 | 68015330 |

Long



| | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|
| Ø mm | 1.9 | 2.35 | 2.95 | 3.55 | 4.15 | 4.75 |
| Order No. | 68015331 | 68015332 | 68015333 | 68015334 | 68015335 | 68015336 |

PrimeTaper Tap



| | | | | | |
|-----------|----------|----------|----------|----------|----------|
| Ø mm | 3.0 | 3.6 | 4.2 | 4.8 | 5.4 |
| Order No. | 68015347 | 68015348 | 68015349 | 68015350 | 68015351 |

Screw taps

PrimeTaper Tap

Stainless steel¹, sterile

- Depth marked 6.5 mm
- Multiple use with option for single use
- Marked with the respective implant diameters

Short



| | | | | | |
|-----------|----------|----------|----------|----------|----------|
| Ø mm | 2.65 | 3.25 | 3.85 | 4.45 | 5.05 |
| Order No. | 68015337 | 68015338 | 68015339 | 68015340 | 68015341 |

Intermediate drills

PrimeTaper Drill

Stainless steel¹, TiN-coated², sterile

- Intermediate drills for fine-tuning the diameter of the osteotomy
- Laser-marked depth indication lines
- Multiple use with option for single use
- Marked with the respective numbers

Long



| | | | | | |
|-----------|----------|----------|----------|----------|----------|
| Ø mm | 2.65 | 3.25 | 3.85 | 4.45 | 5.05 |
| Order No. | 68015342 | 68015343 | 68015344 | 68015345 | 68015346 |

6. Trays

PrimeTaper Surgical Tray

PPSU plastic⁷, silicone⁸ holders, non-sterile

The PrimeTaper Surgical Tray is used during surgery and for storage of PrimeTaper surgical instruments.

- Instruments arranged in order of usage
- Two layers for instruments
- Grommet-less solution for easier cleaning
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains no instruments

Please contact customer service to order PrimeTaper Surgical Kit (surgical tray and necessary instruments)



| | | | |
|-----------|---------------|--------------|----------------|
| Size mm | Length 138 | Width 190 | Height 61.5 |
| Order No. | 68015321 | | |

Upper tray

PrimeTaper Drill long

- Ø1.9 Order no. 68015331
- Ø2.35 Order no. 68015332
- Ø2.95 Order no. 68015333
- Ø3.55 Order no. 68015334
- Ø4.15 Order no. 68015335
- Ø4.75 Order no. 68015336

PrimeTaper Drill short

- Ø1.9 Order no. 68015324
- Ø2.35 Order no. 68015325
- Ø2.95 Order no. 68015326
- Ø3.55 Order no. 68015327
- Ø4.15 Order no. 68015328
- Ø4.75 Order no. 68015329
- Ø5.35 Order no. 68015330

Guide Drill

Order no. 68015133

Implant Driver EV

long


- XS Order no. 68015187
- S Order no. 68015189
- M Order no. 68015191
- L Order no. 68015193

short

- S Order no. 68015188
- M Order no. 68015190
- L Order no. 68015192

PrimeTaper Tap

- Ø3.0 Order no. 68015347
- Ø3.6 Order no. 68015348
- Ø4.2 Order no. 68015349
- Ø4.8 Order no. 68015350
- Ø5.4 Order no. 68015351

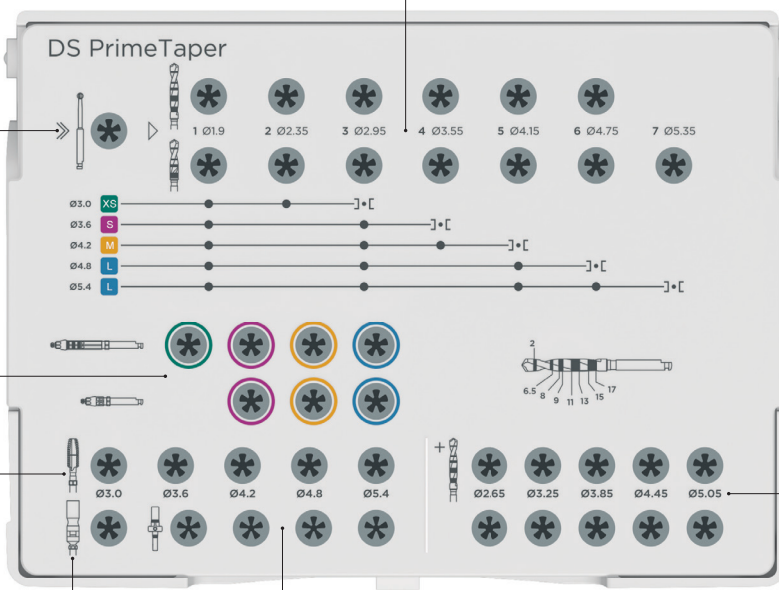

Instrument Extender
Order no. 68015197

PrimeTaper Direction Indicator
Order no. 68015352

Intermediate Drill

short

- Ø2.65 Order no. 68015337
- Ø3.25 Order no. 68015338
- Ø3.85 Order no. 68015339
- Ø4.45 Order no. 68015340
- Ø5.05 Order no. 68015341

long

- Ø2.65 Order no. 68015342
- Ø3.25 Order no. 68015343
- Ø3.85 Order no. 68015344
- Ø4.45 Order no. 68015345
- Ø5.05 Order no. 68015346



Trays


Lower tray

PrimeTaper/Astra Tech
Implant Depth Gauge
Order No. 68015198

Torque Wrench EV
Order No. 25774

Torque Wrench EV
Surgical Driver Handle
Order No. 25775

Hex Driver
Order No. 25772

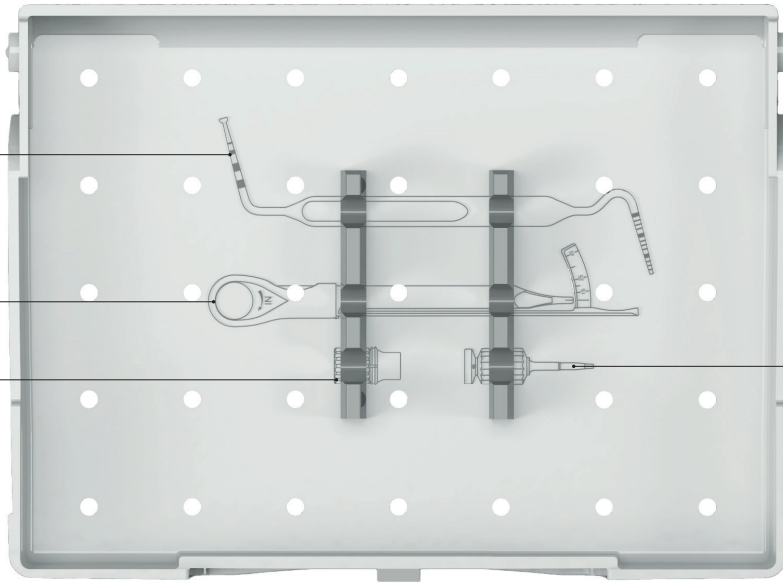

QR code for additional
information about the
surgical tray.



7. Other surgical instruments

Short



| | | | | |
|-----------------|--|----------|----------|----------|
| Total length mm | | 22.9 | 23.0 | 23.1 |
| Order No. | | 68015188 | 68015190 | 68015192 |

Long




| | | | | |
|-----------------|----------|----------|----------|----------|
| Total length mm | 32.3 | 33.0 | 33.2 | 33.3 |
| Order No. | 68015187 | 68015189 | 68015191 | 68015193 |

Implant Driver EV

Stainless steel¹, PEEK², non-sterile

- For picking up and installing implants
- Color coded
- Marked with depth indications and connection size
- Dots to facilitate correct positioning

For use with the contra angle or the Torque Wrench EV Surgical Driver Handle.



The reference point ("0") of the depth markings is the intended bone level, i.e., the lowest point of the bevel.

PrimeTaper Direction Indicator




| | |
|-----------|----------|
| Order No. | 68015352 |
|-----------|----------|

PrimeTaper Direction Indicator

Titanium alloy², non-sterile

- Used after drill ① and drill ③

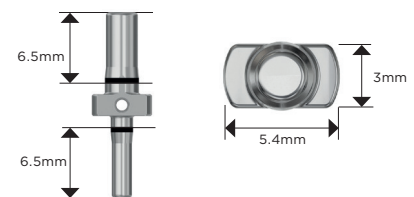

Instrument Extender



| | |
|-----------|----------|
| Order No. | 68015197 |
|-----------|----------|

PrimeTaper/Astra Tech Implant Depth Gauge



| | |
|-----------|----------|
| Order No. | 68015198 |
|-----------|----------|

Instrument Extender

Stainless steel¹, non-sterile

- Used for extending the length of a drill or the Implant Driver EV

PrimeTaper/Astra Tech Implant Depth Gauge

Titanium alloy², non-sterile

- One end corresponds to the implant lengths
- One end is a measuring probe with 0-15 mm markings

Other surgical instruments

Torque Wrench EV

Stainless steel¹, non-sterile

- Used together with the surgical driver handle

Torque Wrench EV Surgical Driver Handle

Stainless steel¹, non-sterile

- Used together with the torque wrench

Torque Wrench EV



| | | |
|-----------|-------|-------|
| Order No. | 25774 | 25775 |
|-----------|-------|-------|

Torque Wrench EV Surgical Driver Handle



Hex Driver

Stainless steel¹, non-sterile

- Used together with a contra angle or the surgical driver handle

Hex Driver



| | | | |
|-----------------|----------|----------|----------|
| Total length mm | 20 | 24 | 35 |
| Order No. | 68015207 | 68015205 | 68015206 |

Hex Driver Manual

Stainless steel¹, non-sterile

Hex Driver Manual



| | | |
|-----------------|-------|-------|
| Total length mm | 20 | 31 |
| Order No. | 25771 | 25772 |

Mucosal Punch

Stainless steel¹, ABS plastic², sterile, single use
QTY 5

Mucosal Punch




| | | | | | | |
|-----------|-------|-------|-------|-------|-------|-------|
| Ø mm | 3.5 | 4 | 4.5 | 5 | 5.5 | 6.5 |
| Order No. | 25711 | 25712 | 25713 | 25714 | 25715 | 25731 |

PrimeTaper Radiographic Template

PC Plastic³, non-sterile

- Planning tool prior to implant surgery
- Used together with the X-ray of the patient's jaw
- Magnification range is from 1.0 to 1.5 presented in two separate sheets

PrimeTaper Radiographic Template

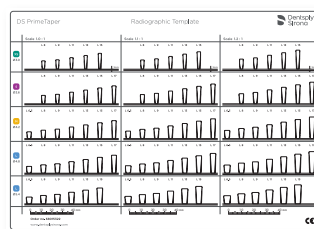

| | |
|-----------|----------|
| Order No. | 68015322 |
|-----------|----------|

8. Instruments - Guided surgery

Specific instruments are available for guided implant installation of DS PrimeTaper implants. They can only be used together with the Simplant SAFE Guide and CEREC Guide 3. Some products are also used for Astra Tech Implant EV, identified through 5-digit order no. When references are made to 6mm depths or lengths, that corresponds to PrimeTaper GS 6.5mm. When using Simplant software or Simplant planning service, case-specific guided surgery instruments can be ordered with the Simplant SAFE Guide.

Punch EV-GS



| | | | |
|-----------|-------|-------|-------|
| Ø mm | 3.6 | 4.2 | 4.8 |
| Order No. | 26010 | 26011 | 26012 |

Initial Drill EV-GS



| | | | |
|-----------|-------|-------|-------|
| Ø mm | 3.6 | 4.2 | 4.8 |
| Order No. | 26013 | 26014 | 26015 |

1-Drill EV-GS



| | | | | | | |
|-------------------|--------|--------|--------|--------|--------|--------|
| Ø mm | 1.9 ND | 1.9 ND | 1.9 ND | 1.9 WD | 1.9 WD | 1.9 WD |
| Implant length mm | 6-8 | 9-11 | 13-15 | 6-8 | 9-11 | 13-15 |
| Order No. | 26051 | 26052 | 26053 | 26060 | 26061 | 26062 |

Punches

Punch EV-GS

Stainless steel[†], sterile

Used to make a circular incision of the implant diameter in the mucosa up to the coronal bone level where the implant shoulder is to be positioned.

- Single use
- Marked with diameter
- Depth marking according to the implant length

Drills

Initial Drill EV-GS

Stainless steel[†], sterile

Used to remove mucosa or to create a centering indentation in the bone for the following drill GS.

- Multiple use
- Marked with diameter
- Depth marking according to the implant length

1-Drill EV-GS

Stainless steel[†], sterile

The first drill for preparing the osteotomy to the planned implant length.

- A drill sleeve is pre-assembled
- Drill: Multiple use
- Sleeve: Single use
- Depth stop
- Guided with the Sleeve-on-Drill system
- Drill sleeve marked with diameter, number and ND for implant Ø3.6mm - Ø4.2mm, WD for implant Ø4.8mm.
- Drills marked with number, length and diameter


PrimeTaper Drill GS

Stainless steel, sterile

The drills are used to prepare the implant site successively to the planned implant length and diameter.

- Multiple use
- Depth stop
- Guided with the Sleeve-on-Drill system
- Marked with the respective number, length and diameter

A drill sleeve is needed and must be ordered separately

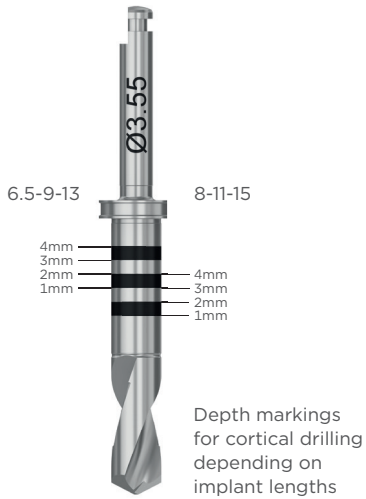


PrimeTaper Drill GS with an attached drill sleeve is also used for the cortical preparation. Use drills 4, 5 and 6 with 6.5-8mm lengths which have the intended depth markings. The drilling depth must be visually controlled when not using the depth stop.

PrimeTaper Drill GS



| | | | | | | |
|-------------------|----------|----------|----------|----------|----------|----------|
| Ø mm | 2.35 | 2.35 | 2.35 | 2.95 | 2.95 | 2.95 |
| Implant length mm | 6.5-8 | 9-11 | 13-15 | 6.5-8 | 9-11 | 13-15 |
| Order No. | 68017229 | 68017230 | 68017231 | 68017232 | 68017233 | 68017234 |

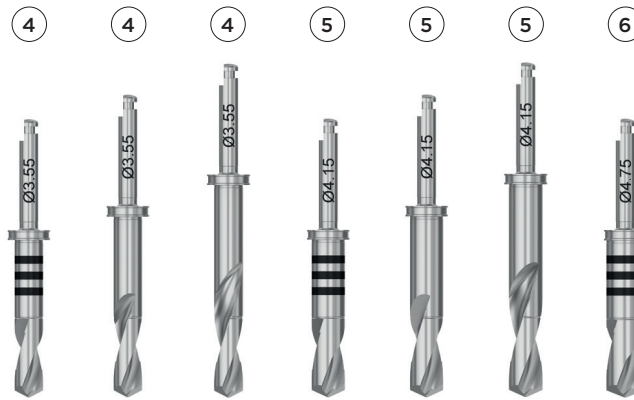

| | | | | | | | |
|-------------------|----------|----------|----------|----------|----------|----------|----------|
| Ø mm | 3.55 | 3.55 | 3.55 | 4.15 | 4.15 | 4.15 | 4.75 |
| Implant length mm | 6.5-8 | 9-11 | 13-15 | 6.5-8 | 9-11 | 13-15 | 6.5-8 |
| Order No. | 68017235 | 68017236 | 68017237 | 68017238 | 68017239 | 68017240 | 68017241 |

PrimeTaper Drill GS



| | | | | | | |
|-------------------|----------|----------|----------|----------|----------|----------|
| Ø mm | 2.65 | 2.65 | 2.65 | 3.25 | 3.25 | 3.25 |
| Implant length mm | 6.5-8 | 9-11 | 13-15 | 6.5-8 | 9-11 | 13-15 |
| Order No. | 68017242 | 68017243 | 68017244 | 68017245 | 68017246 | 68017247 |



| | | | | | | |
|-------------------|----------|----------|----------|----------|----------|----------|
| Ø mm | 3.85 | 3.85 | 3.85 | 4.45 | 4.45 | 4.45 |
| Implant length mm | 6.5-8 | 9-11 | 13-15 | 6.5-8 | 9-11 | 13-15 |
| Order No. | 68017248 | 68017249 | 68017250 | 68017251 | 68017252 | 68017253 |

PrimeTaper Tap GS



| | | | |
|-----------|----------|----------|----------|
| Ø mm | 3.6 | 4.2 | 4.8 |
| Order No. | 68017226 | 68017227 | 68017228 |

Intermediate drills

PrimeTaper Drill GS

Stainless steel¹, sterile

Used for fine-tuning the diameter of the osteotomy.

- Multiple use
- Depth stop
- Guided with the Sleeve-on-Drill system
- Marked with the respective number, length and diameter


Taps

PrimeTaper Tap GS

Stainless steel¹, sterile

Used to tap a thread in very dense bone.

- Multiple use
- Marked with implant diameter
- Markings for tapping depth indication

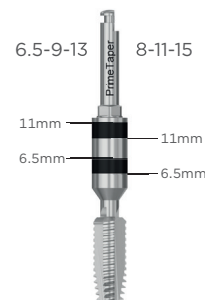

Depth markings for tapping depending on implant lengths.

Sleeves

Sleeve

Stainless steel¹, sterile

For safe guidance of the drills in the surgical guide

- Single use
- Pre-assembled on 1-Drill EV-GS
- Sleeve-on-Drill system
- Marked with ND (Narrow Diameter) when used with drills for implant Ø3.6mm and Ø4.2mm or WD (Wide Diameter) for implant Ø4.8mm
- Marked with Ø1.9 and (1)

1-Sleeve Ø1.9



| | | |
|-----------|-------|-------|
| No. | 1 | 1 |
| Ø | ND | WD |
| Order No. | 26022 | 26027 |

PrimeTaper Drill Sleeve GS

Stainless steel¹, sterile

For safe guidance of the drills in the surgical guide.

- Single use
- Sleeve-on-Drill system
- Marked with ND (Narrow Diameter) when used with drills for implant Ø3.6mm and Ø4.2mm or WD (Wide Diameter) for implant Ø4.8mm
- Marked with the respective diameter and number corresponding to the drills they are used for

[Drill Sleeve is needed and must be ordered separately](#)



PrimeTaper Sleeve GS



| | | | | | | | | |
|-----------|----------|----------|----------|----------|----------|----------|----------|----------|
| No. | 2 | 3 | 3 | 4 | 4 | 5 | 5 | 6 |
| Ø | ND | ND | WD | ND | WD | ND | WD | WD |
| Order No. | 68017254 | 68017255 | 68017256 | 68017257 | 68017258 | 68017259 | 68017260 | 68017261 |



| | | | | | |
|-----------|----------|----------|----------|----------|----------|
| No. | 2½ | 3½ | 4½ | 4½ | 5½ |
| Ø | ND | ND | ND | WD | WD |
| Order No. | 68017262 | 68017263 | 68017264 | 68017265 | 68017266 |


Driver

Implant Driver EV GS


Stainless steel¹, non-sterile

For installing the implant in the prepared implant site.

- Two grooves on the shaft indicate the corresponding implant installation depths 8-11-15 mm and 6.5-9-13mm
- Multiple use
- Color coded



Implant Driver EV GS

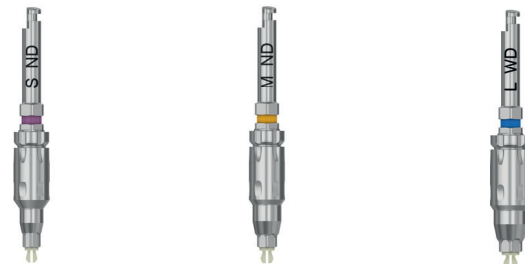

S

M

L

| | | | | | | |
|------------|----------|--|----------|--|----------|--|
| Connection | S | | M | | L | |
| Ø | ND | | ND | | WD | |
| Order No. | 68017001 | | 68017002 | | 68017003 | |

EV-Stabilization Abutment



| | | | | | | |
|-------------------|---------|--------|---------|--------|---------|--------|
| Connection | S | | M | | L | |
| Implant length mm | 8-11-15 | 6-9-13 | 8-11-15 | 6-9-13 | 8-11-15 | 6-9-13 |
| Order No. | 26033 | 26034 | 26035 | 26036 | 26037 | 26038 |

Stabilization Abutment

EV-Stabilization Abutment

Titanium alloy¹, non-sterile

Used to prevent movement of the drilling guide during preparation of the implant site.

- Multiple use
- Marked with diameter and implant length 6-9-13 mm or 8-11-15 mm
- Color coded

Drill for Guide fixation screw



Guide Fixation Screw



| | | |
|-----------|-------|-------|
| | 14mm | Ø2.0 |
| Order No. | 26050 | 26049 |

Guide Fixation

Drill for Guide fixation screw

Stainless steel¹, sterile

Prepare the bone for the fixation screw.

- Multiple use

Guide Fixation Screw

Stainless steel¹, sterile

Secures the guide directly to the bone to avoid guide movement.

- Single use

PrimeTaper Surgical Tray GS



| | | | |
|-----------|---------------|--------------|----------------|
| Size mm | Length 138 | Width 190 | Height 61.5 |
| Order No. | 68017268 | | |

Surgical Tray

PrimeTaper Surgical Tray GS

PPSU¹, silicone² holders, non-sterile

The tray GS is used during surgery and for storage of PrimeTaper surgical instruments.

- Two layers for instruments
- Grommet-less solution for easier cleaning
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains no instruments

Please contact customer service to order PrimeTaper Surgical Kit GS (surgical tray and necessary instruments)

Upper tray

1-Drill EV-GS

- ① Ø1.9 6/6.5-8mm Order No. 26051
- ① Ø1.9 9-11mm Order No. 26052
- ① Ø1.9 13-15mm Order No. 26053

PrimeTaper Drill GS

- ② Ø2.35 6.5-8mm Order No. 68017229
- ② Ø2.35 9-11mm Order No. 68017230
- ② Ø2.35 13-15mm Order No. 68017231
- ③ Ø2.95 6.5-8mm Order No. 68017232
- ③ Ø2.95 9-11mm Order No. 68017233
- ③ Ø2.95 13-15mm Order No. 68017234
- ④ Ø3.55 6.5-8mm Order No. 68017235
- ④ Ø3.55 9-11mm Order No. 68017236
- ④ Ø3.55 13-15mm Order No. 68017237
- ⑤ Ø4.15 6.5-8mm Order No. 68017238
- ⑤ Ø4.15 9-11mm Order No. 68017239
- ⑤ Ø4.15 13-15mm Order No. 68017240
- ⑥ Ø4.75 6.5-8mm Order No. 68017241

Initial Drill EV-GS

- Ø3.6 ND Order No. 26013
- Ø4.2 ND Order No. 26014
- Ø4.8 WD Order No. 26015

Punch EV-GS

- Ø3.6 Order No. 26010
- Ø4.2 Order No. 26011
- Ø4.8 Order No. 26012

Implant Driver EV GS

- (S) ND Order No. 68017001
- (M) ND Order No. 68017002
- (L) WD Order No. 68017003

EV-Stabilization Abutment

- Ø3.6 8-11-15mm Order No. 26033
- Ø3.6 6-9-13mm Order No. 26034
- Ø4.2 8-11-15mm Order No. 26035
- Ø4.2 6-9-13mm Order No. 26036
- Ø4.8 8-11-15mm Order No. 26037
- Ø4.8 6-9-13mm Order No. 26038

Instrument Extender


- Order No. 68015197

Intermediate Drills PrimeTaper GS

- ②½ Ø2.65 6.5-8mm Order No. 68017242
- ②½ Ø2.65 9-11mm Order No. 68017243
- ②½ Ø2.65 13-15mm Order No. 68017244
- ③½ Ø3.25 6.5-8mm Order No. 68017245
- ③½ Ø3.25 9-11mm Order No. 68017246
- ③½ Ø3.25 13-15mm Order No. 68017247
- ④½ Ø3.85 6.5-8mm Order No. 68017248
- ④½ Ø3.85 9-11mm Order No. 68017249
- ④½ Ø3.85 13-15mm Order No. 68017250
- ⑤½ Ø4.45 6.5-8mm Order No. 68017251
- ⑤½ Ø4.45 9-11mm Order No. 68017252
- ⑤½ Ø4.45 13-15mm Order No. 68017253

PrimeTaper Tap GS

- Ø3.6 ND Order No. 68017226
- Ø4.2 ND Order No. 68017227
- Ø4.8 WD Order No. 68017228

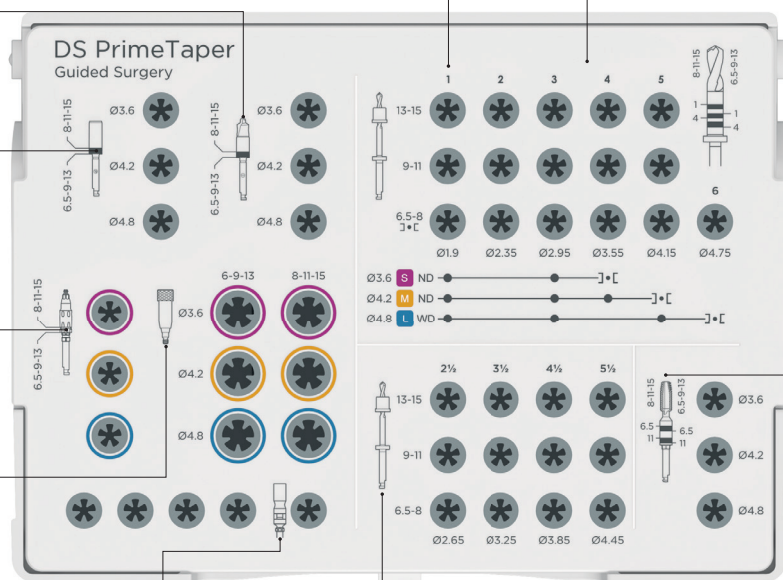


Lower tray

**PrimeTaper/Astra Tech
Implant Depth Gauge**
Order No. 68015198

Torque Wrench EV
Order No. 25774

**Torque Wrench EV
Surgical Driver Handle**
Order No. 25775

Hex Driver
Order No. 25772

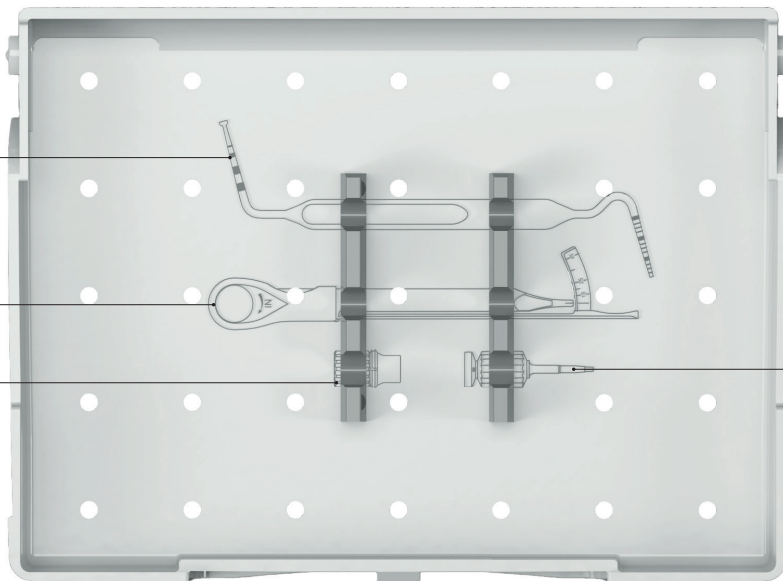

9. Material specifications

Index * will be found at material description for specific products.

Metals

| Type | Index | Composition/Designation | Standard |
|-----------------|-------|--------------------------|-----------|
| Titanium | 1 | Titanium - Grade 4 | ASTM F67 |
| Titanium alloy | 2 | Ti6Al4V | ASTM F136 |
| Stainless steel | 3 | Surgical stainless steel | ASTM F899 |
| TiN Coating | 4 | Titanium Nitride | |
| Aluminum alloy | 5 | AlMg1 | |

Plastics

| Type | Index | Composition/Designation | Standard |
|----------|-------|---------------------------------|----------|
| PEEK | 6 | Polyetheretherketone | |
| PPSU | 7 | Polyphenylsulfone | |
| Silicone | 8 | Polysiloxane | |
| ABS | 9 | Acrylonitrile butadiene styrene | |
| PC | 10 | Polycarbonate | |

10. Index

By order number

| Order No. | page | Order No. | page |
|-----------|--|-----------|---|
| 25711 | Mucosal Punch Ø3.5.....14 | 68011112 | PrimeTaper EV Ø5.4 x 9mm.....5 |
| 25712 | Mucosal Punch Ø4.0.....14 | 68011113 | PrimeTaper EV Ø5.4 x 11mm.....5 |
| 25713 | Mucosal Punch Ø4.5.....14 | 68011114 | PrimeTaper EV Ø5.4 x 13mm.....5 |
| 25714 | Mucosal Punch Ø5.0.....14 | 68011115 | PrimeTaper EV Ø5.4 x 15mm.....5 |
| 25715 | Mucosal Punch Ø5.5.....14 | 68013001 | HealDesign EV (XS) Ø3.5 2.5mm.....7 |
| 25731 | Mucosal Punch Ø6.5.....14 | 68013002 | HealDesign EV (XS) Ø3.5 3.5mm.....7 |
| 25771 | Hex Driver 20mm manual.....14 | 68013003 | HealDesign EV (XS) Ø3.5 4.5mm.....7 |
| 25772 | Hex Driver 31mm manual.....14 | 68013004 | HealDesign EV (XS) Ø3.5 6.5mm.....7 |
| 25774 | Torque Wrench EV.....14 | 68013005 | HealDesign EV (S) Ø4 2.5mm.....7 |
| 25775 | Torque Wrench EV Surgical Driver Handle.....14 | 68013006 | HealDesign EV (S) Ø4 3.5mm.....7 |
| 26010 | Punch EV-GS Ø3.6.....15 | 68013007 | HealDesign EV (S) Ø4 4.5mm.....7 |
| 26011 | Punch EV-GS Ø4.2.....15 | 68013008 | HealDesign EV (S) Ø4 6.5mm.....7 |
| 26012 | Punch EV-GS Ø4.8.....15 | 68013009 | HealDesign EV (S) Ø5 2.5mm.....7 |
| 26013 | Initial Drill EV-GS Ø3.6.....15 | 68013010 | HealDesign EV (S) Ø5 3.5mm.....7 |
| 26014 | Initial Drill EV-GS Ø4.2.....15 | 68013011 | HealDesign EV (S) Ø5 4.5mm.....7 |
| 26015 | Initial Drill EV-GS Ø4.8.....15 | 68013012 | HealDesign EV (S) Ø5 6.5mm.....7 |
| 26022 | 1-Sleeve Ø1.9 Ø ND.....18 | 68013013 | HealDesign EV (S) Ø6 3.5mm.....7 |
| 26027 | 1-Sleeve Ø1.9 Ø WD.....18 | 68013014 | HealDesign EV (S) Ø6 4.5mm.....7 |
| 26033 | EV-Stabilization Abutment, 8-11-15 mm, Ø3.6.....19 | 68013015 | HealDesign EV (M) Ø5 2.5mm.....7 |
| 26034 | EV-Stabilization Abutment, 6-9-13 mm, Ø3.6.....19 | 68013016 | HealDesign EV (M) Ø5 3.5mm.....7 |
| 26035 | EV-Stabilization Abutment, 8-11-15 mm, Ø4.2.....19 | 68013017 | HealDesign EV (M) Ø5 4.5mm.....7 |
| 26036 | EV-Stabilization Abutment, 6-9-13 mm, Ø4.2.....19 | 68013018 | HealDesign EV (M) Ø5 6.5mm.....7 |
| 26037 | EV-Stabilization Abutment 8-11-15mm, Ø4.8.....19 | 68013019 | HealDesign EV (M) Ø6.5 2.5mm.....7 |
| 26038 | EV-Stabilization Abutment 6-9-13mm, Ø4.8.....19 | 68013020 | HealDesign EV (M) Ø6.5 3.5mm.....7 |
| 26049 | Guide Fixation Screw.....19 | 68013021 | HealDesign EV (M) Ø6.5 4.5mm.....7 |
| 26050 | Drill for Guide fixation screw.....19 | 68013022 | HealDesign EV (M) Ø6.5 6.5mm.....7 |
| 26051 | 1-Drill EV-GS Ø1.9 ND 6.5-8mm.....15 | 68013023 | HealDesign EV (L) Ø5 2.5mm.....7 |
| 26052 | 1-Drill EV-GS Ø1.9 ND 9-11mm.....15 | 68013024 | HealDesign EV (L) Ø5 3.5mm.....7 |
| 26053 | 1-Drill EV-GS Ø1.9 ND 13-15mm.....15 | 68013025 | HealDesign EV (L) Ø5 4.5mm.....7 |
| 26060 | 1-Drill EV-GS Ø1.9 WD 6.5-8mm.....15 | 68013026 | HealDesign EV (L) Ø5 6.5mm.....7 |
| 26061 | 1-Drill EV-GS Ø1.9 WD 9-11mm.....15 | 68013027 | HealDesign EV (L) Ø6.5 2.5mm.....7 |
| 26062 | 1-Drill EV-GS Ø1.9 WD 13-15mm.....15 | 68013028 | HealDesign EV (L) Ø6.5 3.5mm.....7 |
| 68010001 | Cover Screw EV (XS).....6 | 68013029 | HealDesign EV (L) Ø6.5 4.5mm.....7 |
| 68010002 | Cover Screw EV (S).....6 | 68013030 | HealDesign EV (L) Ø6.5 6.5mm.....7 |
| 68010005 | Cover Screw EV (M).....6 | 68013031 | HealDesign EV (L) Ø7.5 3.5mm.....7 |
| 68010006 | Cover Screw EV (L).....6 | 68013032 | HealDesign EV (L) Ø7.5 4.5mm.....7 |
| 68011085 | PrimeTaper EV Ø3.0 x 8mm.....5 | 68013039 | HealDesign EV (S) Ø5 3.5mm Triangular.....7 |
| 68011086 | PrimeTaper EV Ø3.0 x 9mm.....5 | 68013040 | HealDesign EV (M) Ø5 3.5mm Triangular.....7 |
| 68011087 | PrimeTaper EV Ø3.0 x 11mm.....5 | 68013041 | HealDesign EV (M) Ø6.5 3.5mm Triangular.....7 |
| 68011088 | PrimeTaper EV Ø3.0 x 13mm.....5 | 68013042 | HealDesign EV (L) Ø5 3.5mm Triangular.....7 |
| 68011089 | PrimeTaper EV Ø3.0 x 15mm.....5 | 68013043 | HealDesign EV (L) Ø6.5 3.5mm Triangular.....7 |
| 68011090 | PrimeTaper EV Ø3.6 x 8mm.....5 | 68013044 | Healing Abutment EV (XS) 2mm.....6 |
| 68011091 | PrimeTaper EV Ø3.6 x 9mm.....5 | 68013045 | Healing Abutment EV (XS) 3mm.....6 |
| 68011092 | PrimeTaper EV Ø3.6 x 11mm.....5 | 68013046 | Healing Abutment EV (XS) 4mm.....6 |
| 68011093 | PrimeTaper EV Ø3.6 x 13mm.....5 | 68013047 | Healing Abutment EV (XS) 6mm.....6 |
| 68011094 | PrimeTaper EV Ø3.6 x 15mm.....5 | 68013048 | Healing Abutment EV (S) 2mm.....6 |
| 68011095 | PrimeTaper EV Ø3.6 x 17mm.....5 | 68013049 | Healing Abutment EV (S) 3mm.....6 |
| 68011096 | PrimeTaper EV Ø4.2 x 6.5mm.....5 | 68013050 | Healing Abutment EV (S) 4mm.....6 |
| 68011097 | PrimeTaper EV Ø4.2 x 8mm.....5 | 68013051 | Healing Abutment EV (S) 6mm.....6 |
| 68011098 | PrimeTaper EV Ø4.2 x 9mm.....5 | 68013052 | Healing Abutment EV (M) 2mm.....6 |
| 68011099 | PrimeTaper EV Ø4.2 x 11mm.....5 | 68013053 | Healing Abutment EV (M) 3mm.....6 |
| 68011100 | PrimeTaper EV Ø4.2 x 13mm.....5 | 68013054 | Healing Abutment EV (M) 4mm.....6 |
| 68011101 | PrimeTaper EV Ø4.2 x 15mm.....5 | 68013055 | Healing Abutment EV (M) 6mm.....6 |
| 68011102 | PrimeTaper EV Ø4.2 x 17mm.....5 | 68013056 | Healing Abutment EV (L) 2mm.....6 |
| 68011103 | PrimeTaper EV Ø4.8 x 6.5mm.....5 | 68013057 | Healing Abutment EV (L) 3mm.....6 |
| 68011104 | PrimeTaper EV Ø4.8 x 8mm.....5 | 68013058 | Healing Abutment EV (L) 4mm.....6 |
| 68011105 | PrimeTaper EV Ø4.8 x 9mm.....5 | 68013059 | Healing Abutment EV (L) 6mm.....6 |
| 68011106 | PrimeTaper EV Ø4.8 x 11mm.....5 | 68015133 | Guide Drill.....8 |
| 68011107 | PrimeTaper EV Ø4.8 x 13mm.....5 | 68015134 | Precision Drill.....8 |
| 68011108 | PrimeTaper EV Ø4.8 x 15mm.....5 | 68015187 | Implant Driver EV (XS) long.....13 |
| 68011109 | PrimeTaper EV Ø4.8 x 17mm.....5 | 68015188 | Implant Driver EV (S) short.....13 |
| 68011110 | PrimeTaper EV Ø5.4 x 6.5mm.....5 | 68015189 | Implant Driver EV (S) long.....13 |
| 68011111 | PrimeTaper EV Ø5.4 x 8mm.....5 | 68015190 | Implant Driver EV (M) short.....13 |

| Order No. | page | Order No. | page |
|-----------|--|-----------|---|
| 68015191 | Implant Driver EV (M) long.....13 | 68017226 | PrimeTaper Tap Ø3.6 ND GS.....17 |
| 68015192 | Implant Driver EV (L) short.....13 | 68017227 | PrimeTaper Tap Ø4.2 ND GS.....17 |
| 68015193 | Implant Driver EV (L) long.....13 | 68017228 | PrimeTaper Tap Ø4.8 WD GS.....17 |
| 68015197 | Instrument Extender.....13 | 68017229 | PrimeTaper Drill 2 Ø2.35 6.5-8mm GS.....16 |
| 68015198 | PrimeTaper/Astra Tech Implant Depth Gauge.....13 | 68017230 | PrimeTaper Drill 2 Ø2.35 9-11mm GS.....16 |
| 68015205 | Hex Driver 24mm.....14 | 68017231 | PrimeTaper Drill 2 Ø2.35 13-15mm GS.....16 |
| 68015206 | Hex Driver 35mm.....14 | 68017232 | PrimeTaper Drill 3 Ø2.95 6.5-8mm GS.....16 |
| 68015207 | Hex Driver 20mm.....14 | 68017233 | PrimeTaper Drill 3 Ø2.95 9-11mm GS.....16 |
| 68015321 | PrimeTaper Surgical Tray.....10 | 68017234 | PrimeTaper Drill 3 Ø2.95 13-15mm GS.....16 |
| 68015322 | PrimeTaper Radiographic Template.....14 | 68017235 | PrimeTaper Drill 4 Ø3.55 6.5-8mm GS.....16 |
| 68015324 | Drill 1 Ø1.9 short.....8 | 68017236 | PrimeTaper Drill 4 Ø3.55 9-11mm GS.....16 |
| 68015325 | PrimeTaper Drill 2 Ø2.35 short.....8 | 68017237 | PrimeTaper Drill 4 Ø3.55 13-15mm GS.....16 |
| 68015326 | PrimeTaper Drill 3 Ø2.95 short.....8 | 68017238 | PrimeTaper Drill 5 Ø4.15 6.5-8mm GS.....16 |
| 68015327 | PrimeTaper Drill 4 Ø3.55 short.....8 | 68017239 | PrimeTaper Drill 5 Ø4.15 9-11mm GS.....16 |
| 68015328 | PrimeTaper Drill 5 Ø4.15 short.....8 | 68017240 | PrimeTaper Drill 5 Ø4.15 13-15mm GS.....16 |
| 68015329 | PrimeTaper Drill 6 Ø4.75 short.....8 | 68017241 | PrimeTaper Drill 6 Ø4.75 6.5-8mm GS.....16 |
| 68015330 | PrimeTaper Drill 7 Ø5.35 short.....8 | 68017242 | PrimeTaper Drill 2½ Ø2.65 6.5-8mm GS.....17 |
| 68015331 | Drill 1 Ø1.9 long.....8 | 68017243 | PrimeTaper Drill 2½ Ø2.65 9-11mm GS.....17 |
| 68015332 | PrimeTaper Drill 2 Ø2.35 long.....8 | 68017244 | PrimeTaper Drill 2½ Ø2.65 13-15mm GS.....17 |
| 68015333 | PrimeTaper Drill 3 Ø2.95 long.....8 | 68017245 | PrimeTaper Drill 3½ Ø3.25 6.5-8mm GS.....17 |
| 68015334 | PrimeTaper Drill 4 Ø3.55 long.....8 | 68017246 | PrimeTaper Drill 3½ Ø3.25 9-11mm GS.....17 |
| 68015335 | PrimeTaper Drill 5 Ø4.15 long.....8 | 68017247 | PrimeTaper Drill 3½ Ø3.25 13-15mm GS.....17 |
| 68015336 | PrimeTaper Drill 6 Ø4.75 long.....8 | 68017248 | PrimeTaper Drill 4½ Ø3.85 6.5-8mm GS.....17 |
| 68015337 | PrimeTaper Drill 2½ Ø2.65 short.....9 | 68017249 | PrimeTaper Drill 4½ Ø3.85 9-11mm GS.....17 |
| 68015338 | PrimeTaper Drill 3½ Ø3.25 short.....9 | 68017250 | PrimeTaper Drill 4½ Ø3.85 13-15mm GS.....17 |
| 68015339 | PrimeTaper Drill 4½ Ø3.85 short.....9 | 68017251 | PrimeTaper Drill 5½ Ø4.45 6.5-8mm GS.....17 |
| 68015340 | PrimeTaper Drill 5½ Ø4.45 short.....9 | 68017252 | PrimeTaper Drill 5½ Ø4.45 9-11mm GS.....17 |
| 68015341 | PrimeTaper Drill 6½ Ø5.05 short.....9 | 68017253 | PrimeTaper Drill 5½ Ø4.45 13-15mm GS.....17 |
| 68015342 | PrimeTaper Drill 2½ Ø2.65 long.....9 | 68017254 | PrimeTaper Sleeve 2 Ø ND GS.....18 |
| 68015343 | PrimeTaper Drill 3½ Ø3.25 long.....9 | 68017255 | PrimeTaper Sleeve 3 Ø ND GS.....18 |
| 68015344 | PrimeTaper Drill 4½ Ø3.85 long.....9 | 68017256 | PrimeTaper Sleeve 3 Ø WD GS.....18 |
| 68015345 | PrimeTaper Drill 5½ Ø4.45 long.....9 | 68017257 | PrimeTaper Sleeve 4 Ø ND GS.....18 |
| 68015346 | PrimeTaper Drill 6½ Ø5.05 long.....9 | 68017258 | PrimeTaper Sleeve 4 Ø WD GS.....18 |
| 68015347 | PrimeTaper Tap Ø3.0.....9 | 68017259 | PrimeTaper Sleeve 5 Ø ND GS.....18 |
| 68015348 | PrimeTaper Tap Ø3.6.....9 | 68017260 | PrimeTaper Sleeve 5 Ø WD GS.....18 |
| 68015349 | PrimeTaper Tap Ø4.2.....9 | 68017261 | PrimeTaper Sleeve 6 Ø WD GS.....18 |
| 68015350 | PrimeTaper Tap Ø4.8.....9 | 68017262 | PrimeTaper Sleeve 2½ Ø ND GS.....18 |
| 68015351 | PrimeTaper Tap Ø5.4.....9 | 68017263 | PrimeTaper Sleeve 3½ Ø ND GS.....18 |
| 68015352 | PrimeTaper Direction Indicator.....13 | 68017264 | PrimeTaper Sleeve 4½ Ø ND GS.....18 |
| 68017001 | Implant Driver EV GS (S).....18 | 68017265 | PrimeTaper Sleeve 4½ Ø WD GS.....18 |
| 68017002 | Implant Driver EV GS (M).....18 | 68017266 | PrimeTaper Sleeve 5½ Ø WD GS.....18 |
| 68017003 | Implant Driver EV GS (L).....18 | 68017268 | PrimeTaper Surgical Tray GS.....19 |

Alphabetical order

| Order No. | | page | Order No. | | page |
|-----------|--|------|-----------|---|------|
| 26051 | 1-Drill EV-GS Ø1.9 ND 6.5-8mm | 15 | 68013059 | Healing Abutment EV (L) 6mm | 6 |
| 26052 | 1-Drill EV-GS Ø1.9 ND 9-11mm | 15 | 68013052 | Healing Abutment EV (M) 2mm | 6 |
| 26053 | 1-Drill EV-GS Ø1.9 ND 13-15mm | 15 | 68013053 | Healing Abutment EV (M) 3mm | 6 |
| 26060 | 1-Drill EV-GS Ø1.9 WD 6.5-8mm | 15 | 68013054 | Healing Abutment EV (M) 4mm | 6 |
| 26061 | 1-Drill EV-GS Ø1.9 WD 9-11mm | 15 | 68013055 | Healing Abutment EV (M) 6mm | 6 |
| 26062 | 1-Drill EV-GS Ø1.9 WD 13-15mm | 15 | 68013048 | Healing Abutment EV (S) 2mm | 6 |
| 26022 | 1-Sleeve Ø1.9 Ø ND | 18 | 68013049 | Healing Abutment EV (S) 3mm | 6 |
| 26027 | 1-Sleeve Ø1.9 Ø WD | 18 | 68013050 | Healing Abutment EV (S) 4mm | 6 |
| 68010006 | Cover Screw EV (L) | 6 | 68013051 | Healing Abutment EV (S) 6mm | 6 |
| 68010005 | Cover Screw EV (M) | 6 | 68013044 | Healing Abutment EV (XS) 2mm | 6 |
| 68010002 | Cover Screw EV (S) | 6 | 68013045 | Healing Abutment EV (XS) 3mm | 6 |
| 68010001 | Cover Screw EV (XS) | 6 | 68013046 | Healing Abutment EV (XS) 4mm | 6 |
| 68015331 | Drill 1 Ø1.9 long | 8 | 68013047 | Healing Abutment EV (XS) 6mm | 6 |
| 68015324 | Drill 1 Ø1.9 short | 8 | 68015207 | Hex Driver 20mm | 14 |
| 26050 | Drill for Guide fixation screw | 19 | 25771 | Hex Driver 20mm manual | 14 |
| 26034 | EV-Stabilization Abutment, 6-9-13mm, Ø3.6 | 19 | 68015205 | Hex Driver 24mm | 14 |
| 26036 | EV-Stabilization Abutment, 6-9-13mm, Ø4.2 | 19 | 25772 | Hex Driver 31mm manual | 14 |
| 26038 | EV-Stabilization Abutment, 6-9-13mm, Ø4.8 | 19 | 68015206 | Hex Driver 35mm | 14 |
| 26033 | EV-Stabilization Abutment, 8-11-15mm, Ø3.6 | 19 | 68015193 | Implant Driver EV (L) long | 13 |
| 26035 | EV-Stabilization Abutment, 8-11-15mm, Ø4.2 | 19 | 68015192 | Implant Driver EV (L) short | 13 |
| 26037 | EV-Stabilization Abutment, 8-11-15mm, Ø4.8 | 19 | 68015191 | Implant Driver EV (M) long | 13 |
| 68015133 | Guide Drill | 8 | 68015190 | Implant Driver EV (M) short | 13 |
| 26049 | Guide Fixation Screw | 19 | 68015189 | Implant Driver EV (S) long | 13 |
| 68013023 | HealDesign EV (L) Ø5 2.5mm | 7 | 68015188 | Implant Driver EV (S) short | 13 |
| 68013024 | HealDesign EV (L) Ø5 3.5mm | 7 | 68015187 | Implant Driver EV (XS) long | 13 |
| 68013042 | HealDesign EV (L) Ø5 3.5mm Triangular | 7 | 68017003 | Implant Driver EV GS (L) | 18 |
| 68013025 | HealDesign EV (L) Ø5 4.5mm | 7 | 68017002 | Implant Driver EV GS (M) | 18 |
| 68013026 | HealDesign EV (L) Ø5 6.5mm | 7 | 68017001 | Implant Driver EV GS (S) | 18 |
| 68013027 | HealDesign EV (L) Ø6.5 2.5mm | 7 | 26013 | Initial Drill EV-GS Ø3.6 | 15 |
| 68013028 | HealDesign EV (L) Ø6.5 3.5mm | 7 | 26014 | Initial Drill EV-GS Ø4.2 | 15 |
| 68013043 | HealDesign EV (L) Ø6.5 3.5mm Triangular | 7 | 26015 | Initial Drill EV-GS Ø4.8 | 15 |
| 68013029 | HealDesign EV (L) Ø6.5 4.5mm | 7 | 68015197 | Instrument Extender | 13 |
| 68013030 | HealDesign EV (L) Ø6.5 6.5mm | 7 | 25711 | Mucosal Punch Ø3.5 | 14 |
| 68013031 | HealDesign EV (L) Ø7.5 3.5mm | 7 | 25712 | Mucosal Punch Ø4.0 | 14 |
| 68013032 | HealDesign EV (L) Ø7.5 4.5mm | 7 | 25713 | Mucosal Punch Ø4.5 | 14 |
| 68013015 | HealDesign EV (M) Ø5 2.5mm | 7 | 25714 | Mucosal Punch Ø5.0 | 14 |
| 68013016 | HealDesign EV (M) Ø5 3.5mm | 7 | 25715 | Mucosal Punch Ø5.5 | 14 |
| 68013040 | HealDesign EV (M) Ø5 3.5mm Triangular | 7 | 25731 | Mucosal Punch Ø6.5 | 14 |
| 68013017 | HealDesign EV (M) Ø5 4.5mm | 7 | 68015134 | Precision Drill | 8 |
| 68013018 | HealDesign EV (M) Ø5 6.5mm | 7 | 68015198 | PrimeTaper/Astra Tech Implant Depth Gauge | 13 |
| 68013019 | HealDesign EV (M) Ø6.5 2.5mm | 7 | 68015352 | PrimeTaper Direction Indicator | 13 |
| 68013020 | HealDesign EV (M) Ø6.5 3.5mm | 7 | 68017229 | PrimeTaper Drill 2 Ø2.35 6.5-8mm GS | 16 |
| 68013041 | HealDesign EV (M) Ø6.5 3.5mm Triangular | 7 | 68017230 | PrimeTaper Drill 2 Ø2.35 9-11mm GS | 16 |
| 68013021 | HealDesign EV (M) Ø6.5 4.5mm | 7 | 68017231 | PrimeTaper Drill 2 Ø2.35 13-15mm GS | 16 |
| 68013022 | HealDesign EV (M) Ø6.5 6.5mm | 7 | 68015332 | PrimeTaper Drill 2 Ø2.35 long | 8 |
| 68013005 | HealDesign EV (S) Ø4 2.5mm | 7 | 68015325 | PrimeTaper Drill 2 Ø2.35 short | 8 |
| 68013006 | HealDesign EV (S) Ø4 3.5mm | 7 | 68017242 | PrimeTaper Drill 2½ Ø2.65 6.5-8mm GS | 17 |
| 68013007 | HealDesign EV (S) Ø4 4.5mm | 7 | 68017243 | PrimeTaper Drill 2½ Ø2.65 9-11mm GS | 17 |
| 68013008 | HealDesign EV (S) Ø4 6.5mm | 7 | 68017244 | PrimeTaper Drill 2½ Ø2.65 13-15mm GS | 17 |
| 68013009 | HealDesign EV (S) Ø5 2.5mm | 7 | 68015342 | PrimeTaper Drill 2½ Ø2.65 long | 9 |
| 68013010 | HealDesign EV (S) Ø5 3.5mm | 7 | 68015337 | PrimeTaper Drill 2½ Ø2.65 short | 9 |
| 68013039 | HealDesign EV (S) Ø5 3.5mm Triangular | 7 | 68017232 | PrimeTaper Drill 3 Ø2.95 6.5-8mm GS | 16 |
| 68013011 | HealDesign EV (S) Ø5 4.5mm | 7 | 68017233 | PrimeTaper Drill 3 Ø2.95 9-11mm GS | 16 |
| 68013012 | HealDesign EV (S) Ø5 6.5mm | 7 | 68017234 | PrimeTaper Drill 3 Ø2.95 13-15mm GS | 16 |
| 68013013 | HealDesign EV (S) Ø6 3.5mm | 7 | 68015333 | PrimeTaper Drill 3 Ø2.95 long | 8 |
| 68013014 | HealDesign EV (S) Ø6 4.5mm | 7 | 68015326 | PrimeTaper Drill 3 Ø2.95 short | 8 |
| 68013001 | HealDesign EV (XS) Ø3.5 2.5mm | 7 | 68017245 | PrimeTaper Drill 3½ Ø3.25 6.5-8mm GS | 17 |
| 68013002 | HealDesign EV (XS) Ø3.5 3.5mm | 7 | 68017246 | PrimeTaper Drill 3½ Ø3.25 9-11mm GS | 17 |
| 68013003 | HealDesign EV (XS) Ø3.5 4.5mm | 7 | 68017247 | PrimeTaper Drill 3½ Ø3.25 13-15mm GS | 17 |
| 68013004 | HealDesign EV (XS) Ø3.5 6.5mm | 7 | 68015343 | PrimeTaper Drill 3½ Ø3.25 long | 9 |
| 68013056 | Healing Abutment EV (L) 2mm | 6 | 68015338 | PrimeTaper Drill 3½ Ø3.25 short | 9 |
| 68013057 | Healing Abutment EV (L) 3mm | 6 | 68017235 | PrimeTaper Drill 4 Ø3.55 6.5-8mm GS | 16 |
| 68013058 | Healing Abutment EV (L) 4mm | 6 | 68017236 | PrimeTaper Drill 4 Ø3.55 9-11mm GS | 16 |

| Order No. | page | Order No. | page |
|-----------|------|---|------|
| 68017237 | 16 | 68011103 | 5 |
| 68015334 | 8 | 68011104 | 5 |
| 68015327 | 8 | 68011105 | 5 |
| 68017248 | 17 | 68011106 | 5 |
| 68017249 | 17 | 68011107 | 5 |
| 68017250 | 17 | 68011108 | 5 |
| 68015344 | 9 | 68011109 | 5 |
| 68015339 | 9 | 68011110 | 5 |
| 68017238 | 16 | 68011111 | 5 |
| 68017239 | 16 | 68011112 | 5 |
| 68017240 | 16 | 68011113 | 5 |
| 68015335 | 8 | 68011114 | 5 |
| 68015328 | 8 | 68011115 | 5 |
| 68017251 | 17 | 68015322 | 14 |
| 68017252 | 17 | 68017254 | 18 |
| 68017253 | 17 | 68017262 | 18 |
| 68015345 | 9 | 68017255 | 18 |
| 68015340 | 9 | 68017256 | 18 |
| 68017241 | 16 | 68017263 | 18 |
| 68015336 | 8 | 68017257 | 18 |
| 68015329 | 8 | 68017258 | 18 |
| 68015346 | 9 | 68017264 | 18 |
| 68015341 | 9 | 68017265 | 18 |
| 68015330 | 8 | 68017259 | 18 |
| 68011085 | 5 | 68017260 | 18 |
| 68011086 | 5 | 68017266 | 18 |
| 68011087 | 5 | 68017261 | 18 |
| 68011088 | 5 | 68015321 | 10 |
| 68011089 | 5 | 68017268 | 19 |
| 68011090 | 5 | 68015347 | 9 |
| 68011091 | 5 | 68015348 | 9 |
| 68011092 | 5 | 68015349 | 9 |
| 68011093 | 5 | 68015350 | 9 |
| 68011094 | 5 | 68015351 | 9 |
| 68011095 | 5 | 68017226 | 17 |
| 68011096 | 5 | 68017227 | 17 |
| 68011097 | 5 | 68017228 | 17 |
| 68011098 | 5 | 26010 | 15 |
| 68011099 | 5 | 26011 | 15 |
| 68011100 | 5 | 26012 | 15 |
| 68011101 | 5 | 25774 | 14 |
| 68011102 | 5 | 25775 | 14 |
| | | PrimeTaper EV Ø4.8 x 6.5mm | 5 |
| | | PrimeTaper EV Ø4.8 x 8mm | 5 |
| | | PrimeTaper EV Ø4.8 x 9mm | 5 |
| | | PrimeTaper EV Ø4.8 x 11mm | 5 |
| | | PrimeTaper EV Ø4.8 x 13mm | 5 |
| | | PrimeTaper EV Ø4.8 x 15mm | 5 |
| | | PrimeTaper EV Ø4.8 x 17mm | 5 |
| | | PrimeTaper EV Ø5.4 x 6.5mm | 5 |
| | | PrimeTaper EV Ø5.4 x 8mm | 5 |
| | | PrimeTaper EV Ø5.4 x 9mm | 5 |
| | | PrimeTaper EV Ø5.4 x 11mm | 5 |
| | | PrimeTaper EV Ø5.4 x 13mm | 5 |
| | | PrimeTaper EV Ø5.4 x 15mm | 5 |
| | | PrimeTaper Radiographic Template | 14 |
| | | PrimeTaper Sleeve 2 Ø ND GS | 18 |
| | | PrimeTaper Sleeve 2½ Ø ND GS | 18 |
| | | PrimeTaper Sleeve 3 Ø ND GS | 18 |
| | | PrimeTaper Sleeve 3 Ø WD GS | 18 |
| | | PrimeTaper Sleeve 3½ Ø ND GS | 18 |
| | | PrimeTaper Sleeve 4 Ø ND GS | 18 |
| | | PrimeTaper Sleeve 4 Ø WD GS | 18 |
| | | PrimeTaper Sleeve 4½ Ø ND GS | 18 |
| | | PrimeTaper Sleeve 4½ Ø WD GS | 18 |
| | | PrimeTaper Sleeve 5 Ø ND GS | 18 |
| | | PrimeTaper Sleeve 5 Ø WD GS | 18 |
| | | PrimeTaper Sleeve 5½ Ø WD GS | 18 |
| | | PrimeTaper Sleeve 6 Ø WD GS | 18 |
| | | PrimeTaper Surgical Tray | 10 |
| | | PrimeTaper Surgical Tray GS | 19 |
| | | PrimeTaper Tap Ø3.0 | 9 |
| | | PrimeTaper Tap Ø3.6 | 9 |
| | | PrimeTaper Tap Ø4.2 | 9 |
| | | PrimeTaper Tap Ø4.8 | 9 |
| | | PrimeTaper Tap Ø5.4 | 9 |
| | | PrimeTaper Tap GS Ø3.6 ND | 17 |
| | | PrimeTaper Tap GS Ø4.2 ND | 17 |
| | | PrimeTaper Tap GS Ø4.8 WD | 17 |
| | | Punch EV-GS Ø3.6 | 15 |
| | | Punch EV-GS Ø4.2 | 15 |
| | | Punch EV-GS Ø4.8 | 15 |
| | | Torque Wrench EV | 14 |
| | | Torque Wrench EV Surgical Driver Handle | 14 |



THE DENTAL
SOLUTIONS
COMPANY™

